



mich\_olg\_third.xml; App=1001.1926; Coh>0.98

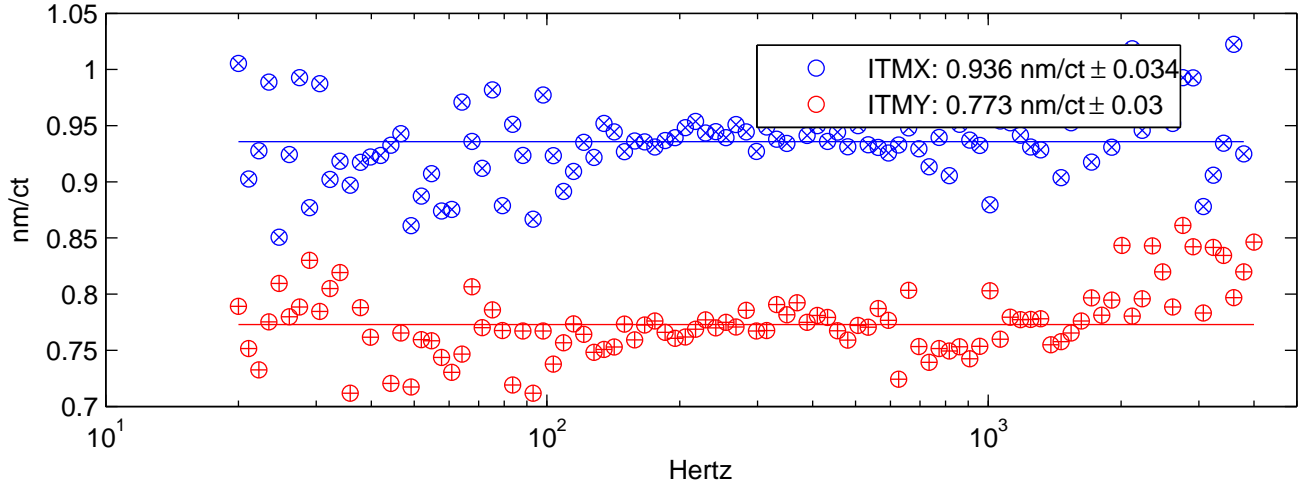

ITMX calibration: N=100 in 20–4000Hz band  
ITMXsweep.xml; f0=0.761 Hz

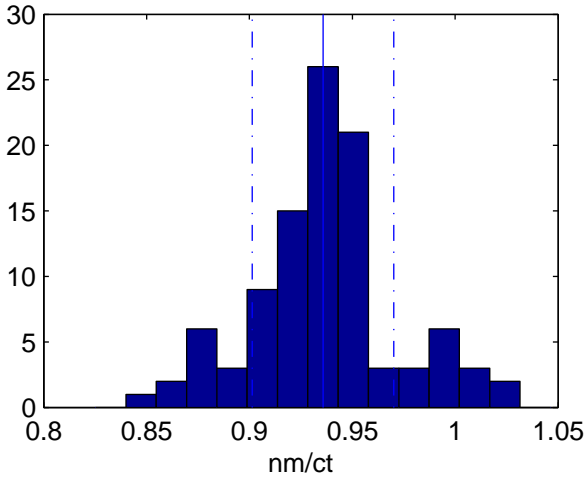

ITMY calibration: N=100 in 20–4000Hz band  
ITMYsweep.xml; f0=0.775 Hz

